Ansell

VALIDATION PACK

BioClean™ Clearview

BCAG, BCAH, BCAP

ansell.com

BioClean™

ref: 1804/BCAG/BCAH/BCAP/VPI6

TABLE OF CONTENTS

BCAG PRODUCT DATASHEET 3
BCAH PRODUCT DATASHEET 6
BCAP PRODUCT DATASHEET 9
EU DECLARATION OF CONFORMITY 12
EU TYPE CERTIFICATE 14
CERTIFICATE OF ANALYSIS 18
CERTIFICATE OF CONFORMITY 19
AUTOCLAVING GOGGLES PROCEDURE 20
AUTOCLAVE TEST RESULTS SUMMARY - ANTI-FOG LENS 22
AUTOCLAVE TEST RESULTS SUMMARY - 40 TO 50 CYCLES 24
IPA TEST SUMMARY 25
QUALITY STATEMENT 26
INSTRUCTIONS FOR USE 27

BIOCLEAN CLEARVIEW
Autoclavable Goggles
BCAG

About

BioClean Clearview Autoclavable Cleanroom Goggles have a super-soft thermoplastic rubber frame to provide wearer comfort and feature upper vents and an indirect lower ventilation system to reduce the risk of contamination entering the controlled environment. These goggles feature a toughened anti-scratch, anti-fog polycarbonate lens for clear vision.

Specifications

MATERIAL:
Thermoplastic rubber frame, toughened polycarbonate lens, latex-free silicone head band with polypropylene hooks

COLOUR:
White frame and black strap

CLASSIFICATION:
EN 166:2001 Optical Class 1

COMPATIBILITY:
ISO Class 4 & EU GMP Grade A

Features

- Toughened, anti-scratch, anti-fog lens
- Super-soft frame
- Upper vents and lower indirect ventilation system
- Non-linting latex-free head band
- Can be worn over eye-glasses
- Tested to withstand 40 autoclave cycles of 30 minutes duration at 121°C/250°F (under laboratory conditions)
- Anti-fog performance remaining for up to 25 cycles with no degradation (under laboratory conditions)

ANTI-FOG LENS

OPTICALLY CORRECT

UPPER VENTS

LOWER INDIRECT VENTS

Quality Standards

- Manufactured in a facility holding ISO 9001:2015
- Processed in an NEBB certified ISO Class 4 cleanroom environment
- Conforms to Category 2 – Personal Protective Equipment Regulation (EU)2016/425
- Complies with requirements of EN 166:2001 standard for personal eye protection

STERILIZATION:
Supplied non-sterile. To be autoclaved at 121°C/250°F for 30 minutes.

Shelf Life & Storage

Five (5) years from date of manufacture. Store in a dry, cool place (<40°C) away from direct sunlight and fluorescent light.

Physical Properties

Total Weight (± 2g)	103g
Lens Thickness (± 0.3mm)	3.1mm
Bridge Width (± 0.5mm)	70mm
Bridge Height (± 0.5mm)	26mm
Overall Width (hinge to hinge)(± 3mm)	190mm
Overall Height (± 3mm)	85mm

Explanation of Markings

REQUIRED MARKINGS	MARKINGS ON FRAME	MEANING
Manufacturer's Identification Mark	BioClean	BioClean™
Standard Number	EN166	European Standard on Personal Eye Protection
Field of Use	BT	Medium energy impact at extremes of temperature
Optical Class	1	High optical quality
Conformity Mark	CE	Conformity with European Standards

TO ORDER

Re-order code	Size
BCAG	Goggle
BCAG-SL	Replacement Lens
BCAG-SS	Replacement Strap

Packing

Goggle (BCAG):
One piece per sealed PE bag (to be removed prior to autoclaving); 12 pieces per box

Replacement Lens (BCAG-SL):
One piece per sealed PE bag; 10 bags per box (10 pieces)

Replacement Strap (BCAG-SS):
25 pieces per sealed PE bag; two bags per box (50 pieces)

For additional information visit us at www.bioclean.com, or call us at:

Nitritex Ltd
Minton Enterprise Park
Oaks Drive
Newmarket, Suffolk
CB8 7YY
United Kingdom

Tel: +44 1638 663338

Ansell US
111 Wood Avenue South
Suite 210
Iselin, NJ 08830
USA

Tel: +1 800 800 0444

Nitritex (M) Sdn.Bhd
2 Jalan Jurunilai U1/20
Seksyen U1,
Hicom Glenmarie Industrial Park
40150 Shah Alam, Selangor
Malaysia

Tel: +603 5569 3857/3859

BCAG/0/PDS45

Neither this document nor any other statement made herein by or on behalf of Ansell should be construed as a warranty of merchantability or that any Ansell product is fit for a particular purpose. Ansell assumes no responsibility for the suitability or adequacy of an end user's selection of goggles for a specific application.

Ansell, ® and ™ are trademarks owned by Ansell Limited or one of its affiliates. © 2012 – 2019 Ansell Limited. All Rights Reserved.

BIOCLEAN CLEARVIEW
Autoclavable Goggles
BCAH

About

Constructed from super-soft, lightweight silicone rubber to provide user comfort and enable prolonged use, BioClean Clearview Autoclavable Cleanroom Goggles feature an indirect ventilation system to reduce the risk of contamination entering the controlled environment, and have an anti-fog polycarbonate lens.

Specifications

MATERIAL:
Silicone rubber frame, polycarbonate lens, latex-free silicone head band with polypropylene hooks

COLOUR:
Translucent white frame and strap

CLASSIFICATION:
No Classification

COMPATIBILITY:
ISO Class 4 & EU GMP Grade A

Features

- Anti-fog lens
- Super-soft frame
- Indirect ventilation system
- Non-linting latex-free head band
- Tested to withstand 50 autoclave cycles of 30 minutes duration at 121°C/250°F (under laboratory conditions)
- Anti-fog performance remaining for up to 25 cycles with no signs of degradation (under laboratory conditions)

ANTI-FOG LENS

SUPER-SOFT FRAME

INDIRECT VENTILATION SYSTEM

Quality Standards

- Manufactured in a facility holding ISO 9001:2015
- Processed in an NEBB certified ISO Class 4 cleanroom environment

STERILIZATION:
Supplied non-sterile. To be autoclaved at 121°C/250°F for 30 minutes.

Shelf Life & Storage

Five (5) years from date of manufacture. Store in a dry, cool place (<40°C) away from direct sunlight and fluorescent light.

Physical Properties

Total Weight (± 2g)	106g
Lens Thickness (± 0.3mm)	1mm
Bridge Width (± 0.5mm)	50mm
Bridge Height (± 0.5mm)	20mm
Overall Width (hinge to hinge)(± 3mm)	180mm
Overall Height (± 3mm)	92mm

Explanation of Markings

REQUIRED MARKINGS	MARKINGS ON FRAME	MEANING
Manufacturer's Identification Mark	BioClean	BioClean™

BCAH PRODUCT DATASHEET

TO ORDER

Re-order code	Size
BCAH	Goggle
BCAH-SL	Replacement Lens
BCAH-SS	Replacement Strap

Packing

Goggle (BCAH):
One piece per sealed PE bag (to be removed prior to autoclaving); 12 pieces per box

Replacement Lens (BCAH-SL):
One piece per sealed PE bag; 10 bags per box (10 pieces)

Replacement Strap (BCAH-SS):
25 pieces per sealed PE bag; two bags per box (50 pieces)

For additional information visit us at www.bioclean.com, or call us at:

Nitritex Ltd
Minton Enterprise Park
Oaks Drive
Newmarket, Suffolk
CB8 7YY
United Kingdom
Tel: +44 1638 663338

Ansell US
111 Wood Avenue South
Suite 210
Iselin, NJ 08830
USA
Tel: +1 800 800 0444

Nitritex (M) Sdn.Bhd
2 Jalan Jurunilai U1/20
Seksyen U1,
Hicom Glenmarie Industrial Park
40150 Shah Alam, Selangor
Malaysia
Tel: +603 5569 3857/3859

BCAH/1907/PDS42

Neither this document nor any other statement made herein by or on behalf of Ansell should be construed as a warranty of merchantability or that any Ansell product is fit for a particular purpose. Ansell assumes no responsibility for the suitability or adequacy of an end user's selection of goggles for a specific application.

Ansell, ® and ™ are trademarks owned by Ansell Limited or one of its affiliates. © 2012 – 2019 Ansell Limited. All Rights Reserved.

BIOCLEAN CLEARVIEW

Autoclavable Panoramic Goggles

BCAP

About

BioClean Clearview Autoclavable Panoramic Goggles have a toughened, anti-scratch, anti-fog lens providing excellent optical clarity even after multiple autoclave cycles. The goggles feature a super-soft frame for comfort and an indirect ventilation system to reduce the risk of contamination entering the controlled environment. The extra wide and deep lens offers the wearer increased field of vision and are ideal for wearing over large eye-glasses.

Specifications

MATERIAL:
Thermoplastic rubber frame, toughened polycarbonate lens, latex-free silicone head band with polypropylene hooks

COLOUR:
White frame and translucent strap

CLASSIFICATION:
EN 166:2001 Optical Class 1

COMPATIBILITY:
ISO Class 4 & EU GMP Grade A

Features

- Toughened anti-scratch, anti-fog lens
- Super-soft frame
- Indirect ventilation system
- Ideal for wearing over eye-glasses
- Non-linting latex-free head band
- Tested to withstand 40 autoclave cycles of 30 minutes duration at 121°C/250°F (under laboratory conditions)
- Anti-fog performance remaining for up to 25 cycles with no degradation (under laboratory conditions)

ANTI-FOG LENS

OPTICALLY CORRECT

INDIRECT VENTILATION SYSTEM

EXTRA WIDE FIELD OF VISION

BCAP PRODUCT DATASHEET

Quality Standards

- Manufactured in a facility holding ISO 9001:2015
- Processed in an NEBB certified ISO Class 4 cleanroom environment
- Conforms to Category 2 – Personal Protective Equipment PPE Regulation (EU)2016/425
- Complies with requirements of EN 166:2001 standard for personal eye protection
- Tested to ANSI/ISEA Z87.1-2010, the American National Standard for Occupational and Educational Personal Eye and Face Protection Devices (BCAP-1 Goggle Style Only)

STERILIZATION:
Supplied non-sterile. To be autoclaved at 121°C/250°F for 30 minutes.

Shelf Life & Storage

Five (5) years from date of manufacture. Store in a dry, cool place (<40°C) away from direct sunlight and fluorescent light.

Physical Properties

Total Weight (± 2g)	103 g
Lens Thickness (± 0.3mm)	2.1mm
Bridge Width (± 0.5mm)	50mm
Bridge Height (± 0.5mm)	25mm
Overall Width (hinge to hinge)(± 3mm)	160mm
Overall Height (± 3mm)	80mm

Explanation of Markings

REQUIRED MARKINGS	MARKINGS ON FRAME	MEANING
Manufacturer's Identification Mark	BioClean	BioClean™
Standard Number	EN166	European Standard on Personal Eye Protection
Field of Use	BT	Medium energy impact at extremes of temperature
Conformity Mark	CE	Conformity with European Standards

BCAP PRODUCT DATASHEET

TO ORDER

Re-order code	Size
BCAP	Goggle
BCAP-1	ANSI Compliant Goggle
BCAP-SL	Replacement Lens
BCAP-SS	Replacement Strap

Packing

Goggle (BCAP & BCAP-1):
One piece per sealed PE bag (to be removed prior to autoclaving); 12 pieces per box

Replacement Lens (BCAP-SL):
One piece per sealed PE bag; 10 bags per box (10 pieces)

Replacement Strap (BCAP-SS):
25 pieces per sealed PE bag; two bags per box (50 pieces)

For additional information visit us at www.bioclean.com, or call us at:

Nitritex Ltd
Minton Enterprise Park
Oaks Drive
Newmarket, Suffolk
CB8 7YY
United Kingdom

Tel: +44 1638 663338

Ansell US
111 Wood Avenue South
Suite 210
Iselin, NJ 08830
USA

Tel: +1 800 800 0444

Nitritex (M) Sdn.Bhd
2 Jalan Jurunilai U1/20
Seksyen U1,
Hicom Glenmarie Industrial Park
40150 Shah Alam, Selangor
Malaysia

Tel: +603 5569 3857/3859

BCAP/1907/PDS38

Neither this document nor any other statement made herein by or on behalf of Ansell should be construed as a warranty of merchantability or that any Ansell product is fit for a particular purpose. Ansell assumes no responsibility for the suitability or adequacy of an end user's selection of goggles for a specific application.

Ansell, ® and ™ are trademarks owned by Ansell Limited or one of its affiliates. © 2012 – 2019 Ansell Limited. All Rights Reserved.

EU DECLARATION OF CONFORMITY

The Manufacturer
NITRITEX (M) SDN BHD,
NO.2, JALAN JURUNILAI U1/20,
SEKSYEN U1, HICOM GLENMARIE
INDUSTRIAL PARK,
40150 SHAH ALAM,
SELANGOR, MALAYSIA

and authorized representative:
NITRITEX LTD
UNIT 4, MINTON ENTERPRISE PARK
OAKS DRIVE, NEWMARKET
SUFFOLK, CB8 7YY, UK

declare under their sole responsibility, that the PPE described hereafter:

BioClean Autoclavable Goggles BCAG

Products manufactured till: [28/05/2024]

PPE to be used against category II risks

is in conformity with the provisions of Regulation (EU) 2016/425 and with the European harmonized standards and is identical to the PPE which is subject to the EU Type Examination; under certificate number 707319 issued by the Notified Body:

BSI (0086)
KITEMARK COURT DAVY AVENUE KNOWLHILL
MILTON KEYNES MK5 8PP UNITED KINGDOM

Guido Van Duren
Director - Regulatory affairs
Ansell

Place: Brussels
Date: 28/05/2019

EU DECLARATION OF CONFORMITY

The Manufacturer
NITRITEX (M) SDN BHD,
NO.2, JALAN JURUNILAI U1/20,
SEKSYEN U1, HICOM GLENMARIE
INDUSTRIAL PARK,
40150 SHAH ALAM,
SELANGOR, MALAYSIA

and authorized representative:
NITRITEX LTD
UNIT 4, MINTON ENTERPRISE PARK
OAKS DRIVE, NEWMARKET
SUFFOLK, CB8 7YY, UK

declare under their sole responsibility, that the PPE described hereafter:

BioClean Autoclavable Goggles BCAP

Products manufactured till: [28/05/2024]

PPE to be used against category II risks

is in conformity with the provisions of Regulation (EU) 2016/425 and with the European harmonized standards and is identical to the PPE which is subject to the EU Type Examination; under certificate number 707319 issued by the Notified Body:

BSI (0086)
KITEMARK COURT DAVY AVENUE KNOWLHILL
MILTON KEYNES MK5 8PP UNITED KINGDOM

Guido Van Duren
Director - Regulatory affairs
Ansell

Place: Brussels
Date: 28/05/2019

EU TYPE CERTIFICATE

bsi.

By Royal Charter

EU Type Examination Certificate

This is to certify that:

Nitritex (M) Sdn Bhd
No.2 Jalan Jurunilai U1/20
Seksyen U1,Hicom Glenmarie Industrial Park
Shah Alam
Selangor
40150
Malaysia

Holds Certificate Number: CE 707319

In respect of:

Safety Eyewear to EN 166:2001
Various models of safety goggles

on the basis that BSI carried out the relevant Type Examination procedures under the requirements with the Regulation (EU) 2016/425 of the European Parliament and Council relating to Personal Protective Equipment Regulation (PPE) Annex V (Module B) and meets the relevant health and safety requirements specified in Annex II

For and on behalf of BSI, a Notified Body for the above Regulation (Notified Body Number 0086):

Chris Lewis - Certification Director, Product Certification

First Issued: 2019-05-28
Latest Issue: 2019-05-28

Effective Date: 2019-05-28
Expiry Date: 2024-05-28

...making excellence a habit.™

EU Type Examination Certificate

No. CE 707319

Product Specification - Goggles

Model: BCGS	BioClean Clearview Goggle BCGS1
Alternative Models:	Bioclean Vijon Goggle BVGS, Bioclean Vijon Goggle BVGS-TV
Product description:	Goggle with polycarbonate lens, polyvinyl chloride frame and elastic strap. Fitted with four ventilation caps.
Technical specifications:	EN 166:2001
EN 166 categorisation:	Optical Class: 1 Field of use: 3 Liquids 4 Large dust particles 9 Molten metals and hot solid BT Medium impact energy at extreme temperatures

Model: BCAP	BioClean Clearview Autoclavable Goggles
Product description	Goggle with polycarbonate lens, thermoplastic rubber (TPR) frame/side shields and ventilation. Fitted with silicone elastic strap, with or without clips.
Technical specifications:	EN 166:2001
EN 166 categorisation:	Optical Class: 1 Field of use: BT Medium impact energy at extreme temperatures

First Issued: 2019-05-28
Latest Issue: 2019-05-28

Effective Date: 2019-05-28
Expiry Date: 2024-05-28

EU Type Examination Certificate

No. CE 707319

Product Specification - Goggles (continued)

Model: BCAG	BioClean Clearview Autoclavable Goggles
Product description:	Goggle with polycarbonate lens, thermoplastic rubber (TPR) frame/side shields and 60% textured polyester and silicone elastic band and ventilation.
Technical specifications:	EN 166:2001
EN 166 categorisation:	Optical Class: 1
	Field of use: BT Medium impact energy at extreme temperatures

First Issued: 2019-05-28
Latest Issue: 2019-05-28

Effective Date: 2019-05-28
Expiry Date: 2024-05-28

EU Type Examination Certificate

No. CE 707319

Certificate Administration Details

Product initially approved on BSI certificate: CE 692742.

Certificate Amendment Record:

Issue Date	Comments	BSI Internal Report Number
May 2019	First issue.	0086:19:9722345

Certificate validity The Certificate holder is responsible for ensuring that the Notified Body is advised of changes to any aspect of the overall process utilised in the manufacture of the product, failure to do so could invalidate the Certificate in respect of product manufactured following the introduction of such changes.

First Issued: 2019-05-28
Latest Issue: 2019-05-28

Effective Date: 2019-05-28
Expiry Date: 2024-05-28

CERTIFICATE OF ANALYSIS

COA
BCAP

Clearview Panoramic
Autoclavable Goggles
(Thermoplastic Rubber)

Certificate of Analysis

Size/Type	Goggle
Lot No.	18-1162
Batch No.	N/A
Expiry Date	03/2023

SAMPLE

Test Data - Sampling Plan

Standard	Plan	AQL	Title	Sample Size	No. of Defects	QC Result
Inhouse	Inhouse	Inhouse	QSP/8.2.4/QA Inspection	10 Boxes	0	Pass
Inhouse	Inhouse	Inhouse	External Packing Conformity	10 Boxes	0	Pass

Analysis Conclusion

This Certificate is based on the evaluation of samples of the above mentioned product and confirms that the product conforms to the specification requirements published by Nitritex Ltd.

This Certificate of Analysis is issued by the authorised signatory below.

Verified by:

Zana

QA Officer

Current product datasheets and Certificates of Irradiation may be downloaded from the BioClean website, www.bioclean.com

CERTIFICATE OF CONFORMITY

COC
BCAP

Clearview Panoramic
Autoclavable Goggles
(Thermoplastic Rubber)

Certificate of Conformity

Size/Type	Goggle
Lot No.	18-1162
Manufacture Date	04/2018
Expiry Date	03/2023
Certificate of Analysis result	Pass

SAMPLE

Declaration of Conformity

The above product is hereby declared as conforming to;

- all technical product specifications
- all manufacturing control specifications
- all applicable standards and regulations specified
- all test parameter ranges as reported on the Certificate of Analysis
- REACH Compliance
- EMEA/410/01 Compliance – as it is declared that this product is free from any animal derived materials (TSE/BSE) and materials derived from genetically modified organisms (GMO)

Issue

This Certificate of Conformity is issued by the authorised signatories on behalf of the authorised supplier.

Verified by:

Zana

QA Officer

Current product datasheets and Certificates of Irradiaton may be downloaded from the BioClean website, www.bioclean.com

Customer Information Aid

Autoclaving Goggles

BioClean™
pure • product • protection

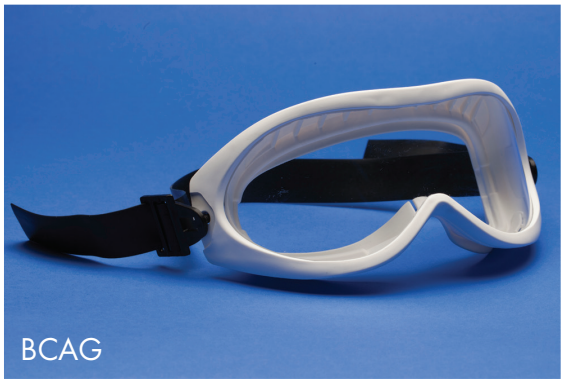

Europe (Headquarters) europe@bioclean.com
Americas americas@bioclean.com
Asia & Middle East malaysia@bioclean.com

www.bioclean.com

Customer Information Aid
Autoclaving Goggles

BioClean™
pure • product • protection

Correct Autoclave Loading

To avoid marks forming on the lenses during the autoclave process, we suggest this procedure is followed.

1 The goggles should be placed in the autoclave bag with the lens vertical (picture A). It does not matter if the straps and clips are next to the lens. Keeping the goggles vertical prevents any condensate from pooling on the lens. The goggles should not be placed horizontally face up (picture B) or face down (picture C) in the autoclave bag.

2 Ensure the autoclave bag is large enough to allow some space between the lens and the plastic part of the bag; doing so will avoid problems arising from condensate being trapped between the lens and the plastic part of the bag.

3 Load the autoclave with the bags paper side down and plastic side up (picture E), otherwise you will get pooling of condensate in the bag. The bags should not be loaded into the autoclave on their edge with the paper 'standing up' (picture F).

Please note:

The steam used in an autoclave should be clean and dry. 'Wet' steam contains suspended droplets of water which add to the condensate without aiding the sterilization process. 'Dry' steam is pure water vapour. The excess condensate from 'wet' steam can push levels beyond the autoclave's capability to dry out the load. Water staining also happens if the load is removed from the autoclave before it has fully cooled and still contains warm, moist air.

With thanks to Westfield Medical Ltd who supplied the autoclave bags. www.westmed.co.uk

Nitritex Ltd, Minton Enterprise Park, Oaks Drive, Newmarket, Suffolk, CB8 7YY, United Kingdom
Tel: +44 (0) 1638 663338 • Fax: +44 (0) 1638 668890 • Email: info@bioclean.com • www.bioclean.com

Autoclave Test Results Summary

BioClean Clearview Autoclavable Goggles with Anti-fog Lens – BCAG-AF, BCAH-AF, BCAP-AF

Goggles are autoclaved at 121°C for 30 minutes per cycle

1. **Test results: BCAG-AF**
   1.1. Lens clarity and anti-fog properties

Autoclave cycles	Lens Clarity	Anti-fog Properties
1-25	Normal	Good
26-30	Normal	Slight fogging*
31-35	Normal	Slight fogging*
36-40	Normal	Slight fogging*

*The intensity of the fog increases with additional autoclave cycles

1.2. Physical condition of goggle accessories

Sample	Condition of the goggle components after 40 autoclave cycles			
	Lens	Housing	Strap	Accessories
1	Normal	Normal	Normal	Normal
2	Normal	Normal	Normal	Normal
3	Normal	Normal	Normal	Normal
4	Normal	Normal	Normal	Normal
5	Normal	Normal	Normal	Normal

2. **Test results: BCAH-AF**
   2.1. Lens clarity and anti-fog properties

Autoclave cycles	Lens Clarity	Anti-fog Properties
1-25	Normal	Good
26-30	Normal	Slight fogging*
31-35	Normal	Slight fogging*
36-40	Normal	Slight fogging*

*The intensity of the fog increases with additional autoclave cycles

2.2. Physical condition of goggle accessories

Sample	Condition of the goggle components after 40 autoclave cycles			
	Lens	Housing	Strap	Accessories
1	Normal	Normal	Normal	Normal
2	Normal	Normal	Normal	Normal
3	Normal	Normal	Normal	Normal
4	Normal	Normal	Normal	Normal
5	Normal	Normal	Normal	Normal

AUTOCLAVE TEST RESULTS SUMMARY- ANTI-FOG LENS

3. Test results: BCAP-AF

3.1. Lens clarity and anti-fog properties

Autoclave cycles	Lens Clarity	Anti-fog Properties
1-25	Normal	Good
26-30	Normal	Slight fogging*
31-35	Normal	Slight fogging*
36-40	Normal	Slight fogging*

*The intensity of the fog increases with additional autoclave cycles

3.2. Physical condition of goggle accessories

Sample	Condition of the goggle components after 40 autoclave cycles			
	Lens	Housing	Strap	Accessories
1	Normal	Normal	Normal	Normal
2	Normal	Normal	Normal	Normal
3	Normal	Normal	Normal	Normal
4	Normal	Normal	Normal	Normal
5	Normal	Normal	Normal	Normal

4. Conclusion

From the tests carried out, there is no visual deterioration on the goggle components (lens, housing, straps, clips) after 40 autoclaving cycles and no impairment on the visibility of the lens.

The BCAG, BCAH and BCAP show no loss of anti-fog integrity up to 25 test cycles; tested in laboratory condition.

AUTOCLAVE TEST RESULTS SUMMARY - 40 TO 50 CYCLES

Autoclave Cycles Summary

BioClean Clearview Autoclavable Goggles– BCAG, BCAH, BCAP

Testing condition: each autoclave cycle is 30 minutes at 121°C

1. Test results

Product	Autoclave cycles tested	Result
BCAG	1-20	Condition unchanged
BCAG	21-40	Minor goggle housing shrinkage
BCAH	1-50	Condition unchanged
BCAP	1-40	Condition unchanged

2. Conclusion

The BCAG and BCAP have been tested to withstand over 40 autoclave cycles; the BCAH have been tested to withstand over 50 autoclave cycles.

IPA 70% Test Results Summary

BioClean Clearview Autoclavable Goggles

1. Test overview

Description	BioClean Clearview Autoclavable Goggle
Product Code	BCAG, BCAH, BCAP
Test Condition	Room Temperature
Test Method	1) Spray IPA (70:30) over assembled goggle 2) Leave assembled goggle to dry completely 3) Assess the lens, housing, strap, clips for physical changes 4) Repeat step 1), 2) & 3) 50 times

2. Test results

Product Code	Number of IPA application cycles observed during test	Observation
BCAG	50	No physical changes detected. Lens, housing, strap and clips compared to standard and condition was good
BCAH	50	No physical changes detected. Lens, housing, strap and clips compared to standard and condition was good
BCAP	50	No physical changes detected. Lens, housing, strap and clips compared to standard and condition was good

3. Conclusion

The BCAG, BCAH and BCAP goggles show no physical changes or deterioration when sprayed with 70% IPA and left to dry 50 times in laboratory conditions.

Product Compliance Statement
BioClean Autoclavable Goggles – BCAH, BCAG and BCAP

Herewith, I confirm that BioClean Autoclavable Goggles – product codes BCAH, BCAG and BCAP –

- are in conformity with the requirements of the Personal Protective Equipment Regulation (EU) 2016/425 and meet the relevant health and safety requirements specified in Annex II;
- are certified to Annex V (Module B) of the regulation by BSI (certificate number CE 707319);
- are processed in a facility operating a Quality Management System compliant with ISO 9001;
- are in conformity with the requirements of EN 166:2001 concerning safety eyewear;
- are processed in a NEBB certified ISO Class 4 cleanroom environment compliant with the requirements of ISO 14644.

Sara Morgan
Quality Specialist – Life Sciences

For more information, contact us:

Manufacturer

Nitritex (M) Sdn Bhd
No.2, Jalan Jurunilai U1/20, Seksyen U1,
Hicom Glenmarie Industrial Park, 40150 Shah Alam,
Selangor, Malaysia

T: +60 3 5569 3857 | F: +60 3 5569 3862

IMPORTER

UK

Nitritex Ltd
Minton Enterprise Park,
Oaks Drive, Newmarket, Suffolk
CB8 7YY, UK

T: +44 1638 663338
F: +44 1638 668890

EU

Ansell Healthcare Europe NV,
Riverside Business Park,
Blvd International, 55
1070 Brussels, Belgium

T: +32 2 528 7400
F: +32 2 528 7401

Australia

Ansell Limited
Level 3, 678 Victoria Street
Richmond , VIC, 3121

T: +61 1800 337 041 | F: +61 1800 803 578

North America Region

Ansell Healthcare Products LLC
111 Wood Avenue South, Suite 210
Iselin, NJ 08830 USA

T: +1 800 800 0444 | F: +1 800 800 0445

Europe, Middle East and Africa (EMEA) Region

Ansell Healthcare Europe NV
Riverside Business Park,
Boulevard International, 55
1070 Brussels, Belgium

T: +32 2 528 74 00 | F: +32 2 528 74 01

Latin America and Caribbean Region

Ansell Commercial México S.A. de C.V.
Blvd. Bernardo Quintana No. 7001-C, Q7001 Torre II.
Suites 1304, 1305 y 1306. Col. Centro Sur, C.P. 76079
Querétaro, Qro. México

T: +52 442 296 2050

Asia Pacific Region

Ansell Global Trading Center (Malaysia) Sdn Bhd
Prima 6, Prima Avenue,
Block 3512, Jalan Teknokrat 6
63000 Cyberjaya, Selangor, Malaysia

T: +60 3 8310 6688 | F: +60 3 8318 6699

Russia

Анселл РУС
123610 Россия, Москва
Краснопресненская
Наб. 12, п.3, оФ 1103

T: +7 495 258 13 16

1902_GOGIFU_V2

Ansell

EN

INSTRUCTIONS FOR USE

BioClean™ Goggles

BioClean goggles are intended to protect the eyes from the following hazards defined by the fields of use in EN 166: 2001

EN 166 Field of use		BCGS1	BVGS	BVGS-TV	BCAG	BCAP	BCAH
3	Liquids	✓	✓	✓	×	×	×
4	Large dust particles	✓	✓	✓	×	×	×
9	Molten metals & hot solids	✓	✓	✓	×	×	×
BT	Medium impact energy at extreme temperatures	✓	✓	✓	✓	✓	×
1	Optical class 1	✓	✓	✓	✓	✓	×
O	Original, non-replaceable ocular	✓	✓	✓	×	×	×

BCGS1 ANSI/ISEA Z87.1 rating: +Impact resistance against flying fragments, objects, large chips, particles, sand, dirt, etc..

Sterilisation

	BCGS1	BVGS	BVGS-TV	BCAG	BCAP	BCAH
Sterile EO	✓	×	×	×	×	×
Sterile Gamma	×	✓	✓	×	×	×
Autoclavable	×	×	×	✓	✓	✓

Recyclable components

	BCGS1	BVGS	BVGS-TV	BCAG	BCAP	BCAH
2 HDPE	Valve	Valve Pouch	Valve Pouch	Pouch	Pouch	Pouch
3 V	Frame	Frame	Frame	–	–	–
5 PP	–	–	–	Side adjusters	Side adjusters	Vents, name plate and locking pin
7 OTHER	Polycarbonate ocular Silicone strap, PE/ PET pouch	Polycarbonate ocular, Silicone strap	Polycarbonate ocular, Silicone strap	SEBS thermoplastic frame, Polycarbonate ocular, Silicone strap	SEBS thermoplastic frame, Polycarbonate ocular, and clip Silicone strap	Polycarbonate ocular and clip, Silicone frame and strap

Explanation of symbols and pictograms used on goggle packaging:

EN166: 2001	Please read the Instructions for Use, prior to using the goggles, or contact Nitritex for more information		Single use only – DO NOT REUSE
CE	Complies with the requirements of the EU PPE Regulation, (EU) 2016/425		Do not use if package is damaged
	Manufacturer	IMPORTER	Importer in EU & UK

The EU Declaration of conformity may be downloaded from:
www.ansell.com/regulatory

EU Type examination carried out by:
BSI Assurance UK Ltd, Kitemark Court, Davy Avenue, Knowlhill, Milton Keynes, MK5 8PP, UK
Notified Body Number 0086

Warnings!

- Eye-protectors against high speed particles worn over standard ophthalmic spectacles may transmit impacts, thus creating a hazard to the wearer.
- If protection against high speed particles at extremes of temperature is required then the selected eye-protector should be marked with the letter T immediately after the impact letter, i.e. FT, BT or AT. If the impact letter is not followed by the letter T then the eye protector shall only be used against high speed particles at room temperature.
- Materials that come into contact with the wearer's skin could cause allergic reactions to susceptible individuals.
- Scratched or damaged oculars should be replaced (BCAG, BCAH and BCAP only).
- To maintain the safety and effectiveness of the goggles they must be stored and transported in their original packaging.
- BCAG, BCAH and BCAP, remove goggles from bag prior to autoclaving.

Cleaning BCAP, BCAG & BCAH Goggles

Instructions for reprocessing BCAP, BCAG and BCAH goggles can be downloaded from
www.bioclean.com/catalogues/Autoclaving Goggles Procedure.pdf

Use only de-ionised or distilled water when autoclaving, autoclave at 121°C (250°F) for 30 minutes only.
BCGS1, BVGS and BVGS-TV are single use and must not be reprocessed.

Replacement parts

	BCGS1	BVGS	BVGS-TV	BCAG	BCAP	BCAH
Ocular	×	×	×	BCAG-SL	BCAP-SL	BCAH-SL
Strap	×	×	×	BCAG-SS	BCAP-SS	BCAH-SS

To change the ocular or strap on a goggle, simply unclip the original part and clip the replacement into its place. For ocular replacement ensure that the edge of the ocular is fully enclosed by the frame and any clips are replaced securely.

Ansell

Contact your Ansell representative for ordering or more information.

North America
US Tel: 800 952 9916
CA Tel: 1-844-494-7854
Email: info@ansell.com

Central & South America
Tel: +52(442) 296 2050
Email: cslac@ansell.com

Brazil
Tel: +55-11-3356-3100
Email: luvas.medicas@ansell.com

Europe, Middle East & Africa
Tel: +32 (0)2528 7400
Email: info@ansell.eu

Asia Pacific
Tel: +603 8310 6688
Email: apac.medical@ansell.com

Australia & New Zealand
Tel: +61 3 9270 7270
Email: protection@ap.ansell.com

ansell.com

Ansell, ® and ™ are trademarks owned by Ansell Limited or one of its affiliates.
© 2019 Ansell Limited. All Rights Reserved.